

ANALIZA BIAŁEK



Scan for verify



100018022

Laboratory of Analysis

Client: Anonymous
Order number: 100018022
Name: SELLIZA NANDROL P
Number of samples: 1 ampoule

Batch number: 0S25P3412
Receive date: 2026-09-03
Start date: 2026-09-11
End date: 2026-09-13

Sample identification

Substance	Method of taking a sample	Form
Nandrolone Phenylpropionate	Sample provided by customer	Transparent liquid in a glass ampoule

Results

Substance	Sample name	Content	Purity
Nandrolone Phenylpropionate	SELLIZA NANDROL P 100MG	93,58mg/ml	-----

Research comment

The test sample was applied in the amount of 3 μ l to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H₂O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peak of the sought substance appeared. Its content, when compared to the reference chromatogram, is 93,58mg/ml. Height the measurement error is +-1mg. The actual state of the sample sent before the test is presented on the photo below.

Photo of the test sample




Password

USB20UOV

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajac



ANALIZA BIAŁEK




Scan for verify



100018022

Chromatogram

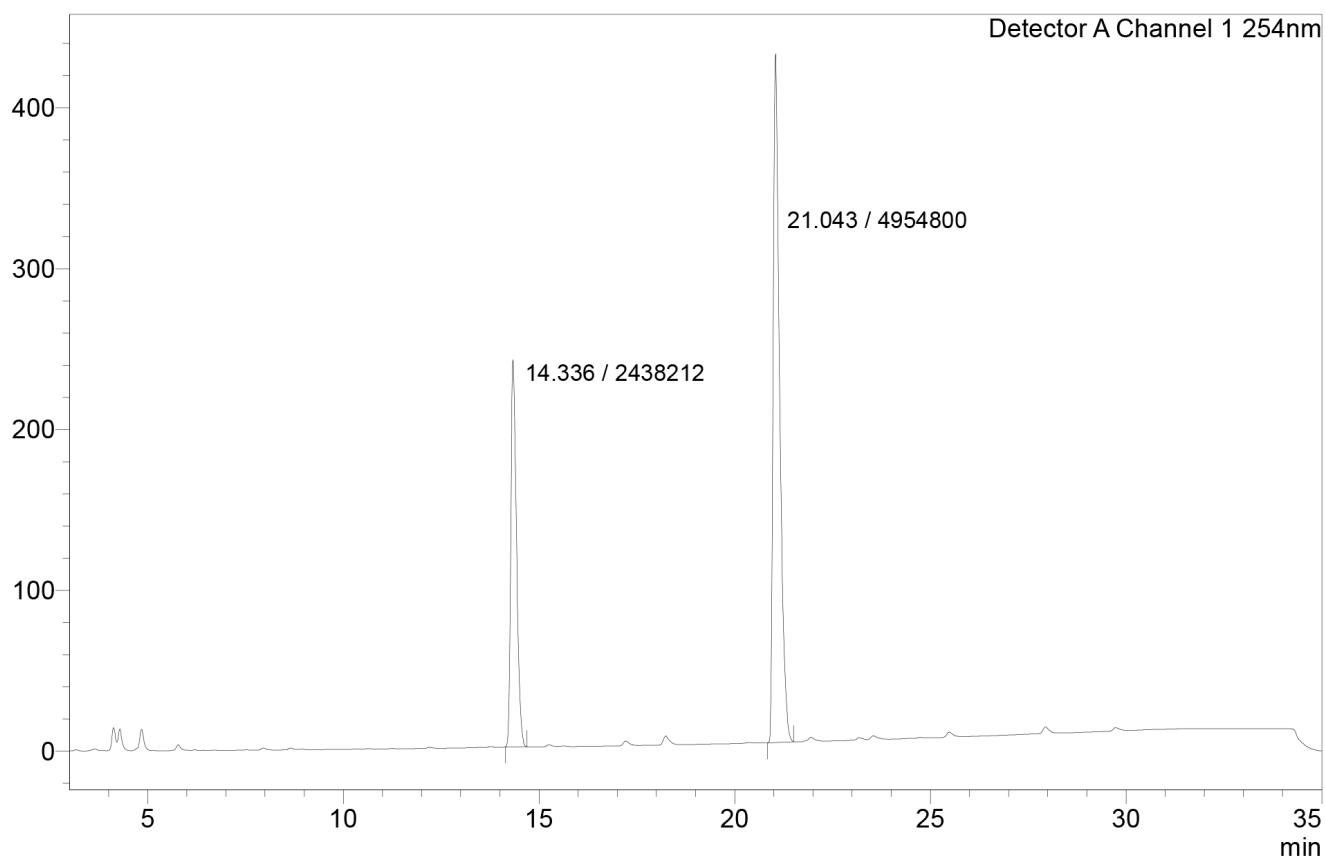

Method

Time	H2O + 0,1% TFA	ACN + 0,1% TFA
0min	60%	40%
2min	60%	40%
27min	5%	95%
30min	5%	95%

Password

USB20UOV

Analiza Bialek sp. z o.o.

KRS: 0000966168

NIP: 8992922970

REGON: 521751875

Headquarters and Laboratory:

ul. Duńska 9, 54-427 Wrocław

Budynek DELTA

Lab technician:

Analysis and research specialist

mgr Arkadiusz Zajac